

Metriso[®] B530 Basic (Part No.: 7100.B530.MK)

- Suitable for resistance to ground and point-to-point resistance measurements according to IEC 61340-4-1 Ed. 2.0 and IEC 61340-2-3
- Suitable for measuring the electrical resistance of footwear and flooring in combination with a person according to IEC 61340-4-5.
- Low ohmic measurement range 1Ω - $10k\Omega$ to measure the resistance of grounded objects
- Digital and analog display with bar graph or pointer
- Optical Indicator LED red and green for voltage measuring range
- Optical Indicator LED red for Test/Measuring
- Includes two Probes Model 870 according to IEC 61340-4-1 Ed. 2.0 / IEC 61340-2-3 extension and a handheld probe according to IEC 61340-4-5



Probe Modell 870



Extension for Probe 870



Handheld probe Model 45

Technical Information

Page 2 of 3

Part No.: 7100.B530.MK



♦ Untere Gießwiesen 21 ♦ 78247 Hilzingen ♦ Tel.: +49-7731-86880 ♦ Fax: +49-7731-868830

Technical data:

Test voltage: DC 10V, 100V, 500V
Test range Resistance: 1 Ω bis 199 G Ω
Operation: Battery operated
Probe: 2 x Model 870
1 x Handheld probe Model 45
1 x Extension for Probe 870
Size: 225 x 130 x 140 mm (WxHxD)
Weight (complete KIT): 9 kg

Supplied with:

- Digital high resistance tester Metriso B530
- Connecting cables
- User's manual in German / English
- 2 probes Model 870 acc. to IEC 61340-4-1/2-3
- 1 handheld probe Model 45 acc. to IEC 61340-4-5
- 1 Extension for Probe 870
- Conductive carrying case

Technical specifications

Meas. Qty.	U _M ²			Range	Measuring Range	Resolution	Intrinsic Uncertainty ¹	Measuring Uncertainty	Overload Capacity
RES D	10 V ³			10 kΩ	1,0 kΩ ... 9,99 kΩ	0,01 k	±(5% rdg. + 10 d)	±(7% rdg. + 10 d)	500 V AC/DC TRMS
				100 kΩ	10,0 kΩ ... 99,9 kΩ	0,1 k	±(5% rdg. + 3 d) ⁵	±(7% rdg. + 3 d)	
				1 MΩ ⁴	100 kΩ ... 999 kΩ	1 k	±(5% rdg. + 3 d)	±(7% rdg. + 3 d)	
	100 V ³	500 V ³	10 MΩ	1,00 MΩ ... 9,99 MΩ	10 k	±(5% rdg. + 3 d)	±(7% rdg. + 3 d)		
			100 MΩ	10,0 MΩ ... 99,9 MΩ	100 k	±(5% rdg. + 3 d)	±(7% rdg. + 3 d)		
			1 GΩ	100 MΩ ... 999 MΩ	1 M	±(5% rdg. + 3 d)	±(7% rdg. + 3 d)		
			10 GΩ	1,00 GΩ ... 9,99 GΩ	10 M	±(5% rdg. + 3 d)	±(10% rdg. + 3 d)		
			100 GΩ	10,0 GΩ ... 99,9 GΩ	100 M	±(8% rdg. + 3 d)	±(10% rdg. + 3 d)		
			200 GΩ	100 GΩ ... 199 GΩ	1 G	±(15% rdg. + 5 d)	±(25% rdg. + 20 d)		
U AC/DC				100 V	10,0 V ... 99,9 V	0,1 V	±(2,5% rdg. + 3 d)	±(5% rdg. + 3 d)	500 V AC/DC TRMS
				500 V	100 V ... 499 V	1 V			
R	Display range as of 01,0 Ω			100 Ω	1,0 ... 99,9 Ω	0,1 Ω	±(2,5% rdg. + 3 d)	±(5% rdg. + 3 d)	500 V AC/DC TRMS
				1 kΩ	100 ... 999 Ω	1 Ω			
				10 kΩ	1,00 ... 9,99 kΩ	10 Ω			

- 1 year limited warranty
- Recommended calibration interval: 2 years


Technical Information

Page 3 of 3


Part No.: 7100.B530.MK

♦ Untere Gießwiesen 21 ♦ 78247 Hilzingen ♦ Tel.: +49-7731-86880 ♦ Fax: +49-7731-868830


Possible measurements with the MetrISO 3000 Test-Kit

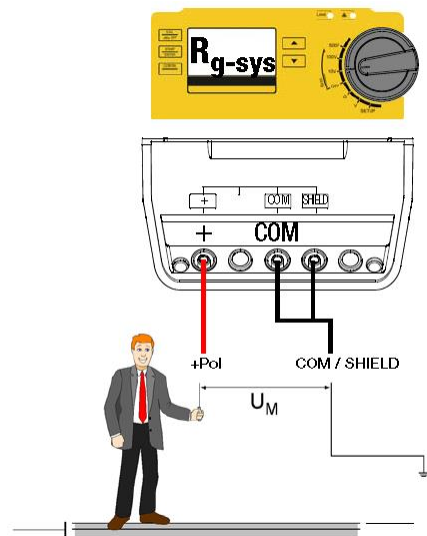

$R_{G \text{ system}}$
Resistance of person /
ESD shoes / flooring to ground

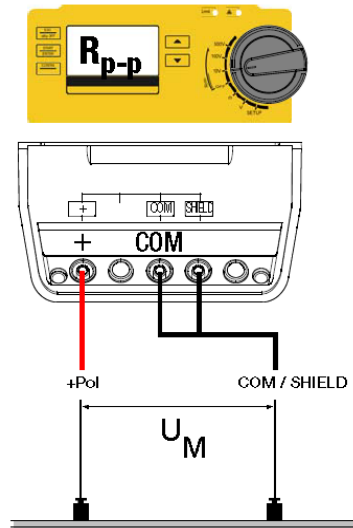

R_{p-p}
Point to Point Resistance

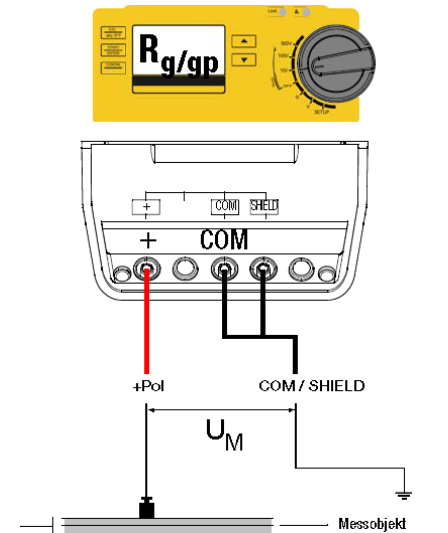

R_G
Resistance to ground or groundable
point

Optional:

Part No.: 7100.TF530

Digital Thermo-Hygrometer

